H836 Hydrogen

Specification Sheet



0.0001** to 2.5 mg (1 g sample) **Instrument Range***

Precision[†] 0.00005 mg or 2% RSD, whichever is greater

Analysis Time 90 seconds (including outgas, purge, and analysis delay)

180 seconds (nominal) **Cycle Time**

Calibration Standards (single or multi-point); manual; gas dose

Sample Size 1 g (nominal)

Detection Method Non-Dispersive Infrared Absorption

• Anhydrous Magnesium Perchlorate (MgClO₄) **Chemical Reagents** • Oxygen/Moisture Indicating Tube

· Sodium Hydroxide on an Inert Base

• Copper Oxide, Copper Turnings

Gas Requirements

He: (99.99% pure), 22 psi (1.5 bar) ±5% Ar: (99.999% pure), 22 psi (1.5 bar) ±5% Carrier:

Pneumatic: Compressed Air, 40 psi (2.8 bar) $\pm 10\%$, source must be oil and water free

Gas Flow Rates

Carrier: 460 cc/minute Pneumatic: 280 cc/analysis

Furnace Impulse furnace with current and power control 7500 Watts maximum, liquid cooled

Coolant 3.2 L LECO Coolant

Operating Conditions

15 to 35°C (59 to 95°F) **Temperature** Rel. Humidity 20 to 80%, non-condensing

Dimensions^{††}

Height: 36 in. (91.5 cm) nominal; 39.25 in. (100 cm) with load head cover lift engaged

Width: 27.75 in. (71 cm)

Depth: 30 in. (76 cm) without monitor; 31.5 in. (80 cm) with attached touch-screen monitor

Electrical Power 230 V~ (+10/-15%; at max load); 50A, 50/60 Hz, Single Phase; 12,500 BTU/hr[‡]

Weight (approximate) Analyzer: 410 lb. (186 kg) without touch-screen monitor



^{*}Use the following formula to calculate element concentration:

[%] element concentration = ((absolute element mass in mg)/(sample mass in mg))*100

^{**}Lower range is calculated as 2 σ instrument blank deviation. Method range may differ due to factors such as sample type and method parameters.

 $^{^{\}dagger}$ Calculated as 1 $_{\odot}$ instrument blank deviation. Method precision may differ due to sample inhomogeneity or other external factors.

^{tt}Allow for a 6 in. (15 cm) minimum access area around all sides.

[‡]Average output based on nominal operating parameters.

V~ denotes VAC.

Part Numbers


H836-MC	H w/PC and touch-screen
H836-C	H w/PC
H836-HC	H w/PC and autocleaner
H836-HMC	H w/PC, touch-screen, and autocleaner

Theory of Operation

The H836 Hydrogen system is designed for wide-range measurement of hydrogen content of steel, refractory metals, and other inorganic materials. The instrument features custom MS Windows®-based software designed specifically for touch operation.

A pre-weighed sample is placed in a graphite crucible which is then heated in an impulse furnace to release analyte gases. An inert gas carrier, typically helium, sweeps the liberated analyte gases out of the furnace and through a Mass Flow Controller to a detector. Oxygen present in the sample reacts with the graphite crucible to form CO and CO₂, which flows through a heated reagent, where the CO is oxidized to form CO₂, and H₂ is oxidized to form H₂O. The gas then continues through a NDIR cell where H₂O is detected. These analytes are then scrubbed out of the carrier gas stream.

The detection system is comprised of a single NDIR detector. NDIR cells are based on the principle that H₂O absorbs infrared (IR) energy at unique wavelengths within the IR spectrum. Incident IR energy at these wavelengths is absorbed as the gases pass through the IR absorption cells. The concentration of an unknown sample is determined relative to calibration standards. To reduce interferences from instrument drift, NDIR reference measurements of pure carrier gas are made prior to each analysis.

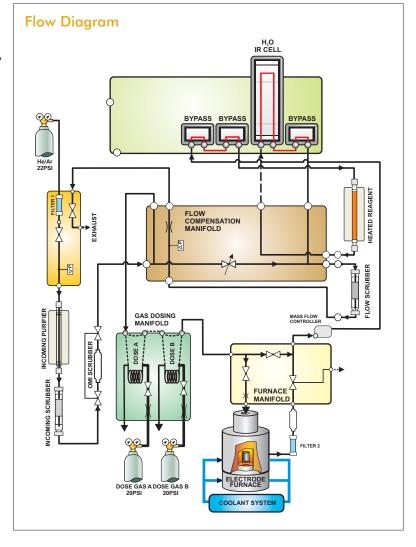

Specifications and part numbers may change. Consult LECO for latest information

LECO Corporation 3000 Lakeview Avenue • St. Joseph, MI 49085 • Phone: 800-292-6141 • Fax: 269-982-8977

